



iCell[®] Cardiomyocytes²

User's Guide

Document ID: X1001



Restrictions and Liabilities

This document is provided "as is." FUJIFILM Cellular Dynamics, Inc. (FCDI), assumes no responsibility for any typographical, technical, or other inaccuracies in this document. FCDI reserves the right to periodically change information that is contained in this document; however, FCDI makes no commitment to provide any such changes, updates, enhancements, or other additions to this document to you in a timely manner or at all.

OTHER THAN THE EXPRESS LIMITED WARRANTY SET FORTH IN WWW.FUJIFILMCDI.COM/PRODUCT-WARRANTY/, FCDI MAKES NO, AND DISCLAIMS ALL, REPRESENTATIONS, WARRANTIES, CONDITIONS OR COVENANTS, EXPRESS OR IMPLIED, WITH RESPECT TO ANY PRODUCT REFERENCED HEREIN OR PERFORMANCE OF ANY SERVICES REFERENCED HEREIN, INCLUDING BUT NOT LIMITED TO, ANY EXPRESS OR IMPLIED WARRANTIES OR CONDITIONS OF FITNESS FOR A PARTICULAR PURPOSE, NON-INFRINGEMENT, MERCHANTABILITY, DURABILITY, TITLE, OR RELATED TO THE PERFORMANCE OR NON-PERFORMANCE OF ANY PRODUCT REFERENCED HEREIN OR PERFORMANCE OF ANY SERVICES REFERENCED HEREIN).

This document might contain references to third-party sources of information, hardware or software, products or services and/or third-party websites (collectively the "Third-Party Information"). FCDI does not control, and is not responsible for, any Third-Party Information, including, without limitation the content, accuracy, copyright compliance, compatibility, performance, trustworthiness, legality, decency, links, or any other aspect of Third-Party Information. The inclusion of Third-Party Information in this document does not imply endorsement by FCDI of the Third-Party Information or the third party in any way.

FCDI does not in any way guarantee or represent that you will obtain satisfactory results from using iCell Cardiomyocytes² as described herein. The only warranties provided to you are included in the Limited Warranty set forth in www.fujifilmcdi.com/product-warranty/. You assume all risk in connection with your use of iCell Cardiomyocytes².

Conditions of Use

iCell Cardiomyocytes² are FOR RESEARCH USE ONLY and NOT FOR THERAPEUTIC USE. See www.fujifilmcdi.com/warranty/ for USE RESTRICTIONS applicable to the cells and other terms and conditions related to the cells and their use.

Trademarks

iCell and MyCell are registered trademarks, and Cellular Dynamics and the  logo are trademarks of FUJIFILM Cellular Dynamics, Inc. and may not be used without the express written permission of FUJIFILM Cellular Dynamics, Inc.

All other brands, product names, company names, trademarks, and service marks are the properties of their respective owners.

Origin

iCell Cardiomyocytes² are manufactured in the United States of America.

Copyright Notice

© 2018 FUJIFILM Cellular Dynamics, Inc. All rights reserved. This document may not be reproduced, distributed, modified or publicly displayed without the express written permission of FUJIFILM Cellular Dynamics, Inc.

Revision History

Document ID: X1001
Version 2.0: September 2020

Table of Contents

Before You Begin	ii
Chapter 1. Introduction	1
Components Supplied by FUJIFILM Cellular Dynamics	2
Required Equipment and Consumables	2
Technical Support, Knowledge Base, and Training	3
Workflow Diagram	4
Chapter 2. Handling and Storage	5
Handling iCell Cardiomyocytes ²	5
Handling iCell Cardiomyocytes Media	5
Chapter 3. Preparing Cell Culture Surfaces	6
Chapter 4. Thawing Media	7
Chapter 5. Thawing iCell Cardiomyocytes²	8
Chapter 6. Plating iCell Cardiomyocytes²	10
Chapter 7. Maintaining iCell Cardiomyocytes²	11

Before You Begin

Notes

- Immediately transfer the frozen vials to liquid nitrogen storage.
- Read this entire User's Guide before handling or using iCell® Cardiomyocytes².
- iCell Cardiomyocytes² are FOR RESEARCH USE ONLY and NOT FOR THERAPEUTIC USE. See www.fujifilmcdi.com/warranty/ for USE RESTRICTIONS applicable to the cells and other terms and conditions related to the cells and their use.
- A Safety Data Sheet (SDS) for dimethyl sulfoxide (DMSO), in which iCell Cardiomyocytes² are frozen, is available online at www.fujifilmcdi.com/lit/ or on request from FUJIFILM Cellular Dynamics. Only technically qualified individuals experienced in handling DMSO and human biological materials should access, use, or handle iCell Cardiomyocytes².

Chapter 1. Introduction

iCell Cardiomyocytes² from FUJIFILM Cellular Dynamics, Inc. (FCDI), are highly purified, human cardiomyocytes derived from induced pluripotent stem (iPS) cells using FCDI's proprietary differentiation and purification protocols. iCell Cardiomyocytes² are a mixture of spontaneously electrically active atrial-, nodal-, and ventricular-like myocytes with typical biochemical, electrophysiological, and mechanical characteristics and expected responses upon exposure to exogenous agents. Thus, these cells provide a reliable source of human cardiomyocytes suitable for use in targeted drug discovery, toxicity testing, and other life science research.

When thawed and plated with iCell Cardiomyocytes Plating Medium and maintained in iCell Cardiomyocytes Maintenance Medium as instructed in this User's Guide, iCell Cardiomyocytes² will begin to beat spontaneously within 24 hours. When seeded at appropriate densities, iCell Cardiomyocytes² also will form electrically connected syncytial layers that beat in synchrony and can be used for electrophysiology interrogation via such techniques as microelectrode array and impedance measurements on day 4 post-thaw.

iCell Cardiomyocytes Maintenance Medium is antibiotic-free and has been specially formulated to maintain the health and function of the cardiomyocytes while limiting the proliferation of the small percentage of non-cardiomyocyte cells. iCell Cardiomyocytes² therefore can be maintained in culture for at least 14 days in the Maintenance Medium without appreciable loss of purity, enabling longer term studies. Thus, the combination of FCDI's purification process and adherence to the procedures described in this User's Guide makes additional use of antibiotics unnecessary.

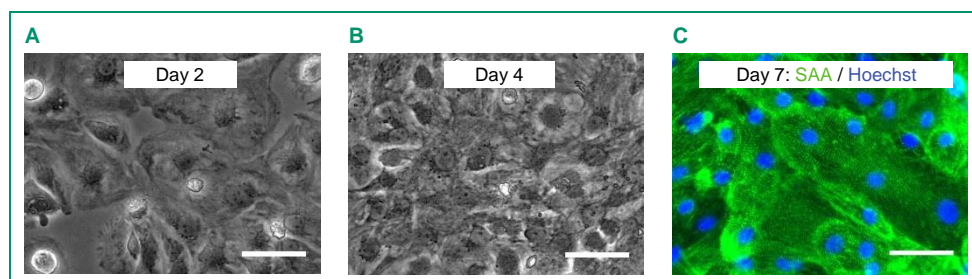


Figure 1: iCell Cardiomyocytes² Represent a Highly Pure Population of Human Myocytes

These example images show iCell Cardiomyocytes² at days 2, 4 and 7 post-plating. The cells form a syncytial layer in culture within 4 days post-plating and show the appropriate cardiac markers as demonstrated by immunocytochemistry: sarcomeric alpha-actinin (SAA, green) and Hoechst (blue). Scale bar = 50 μ m.

Components Supplied by FUJIFILM Cellular Dynamics

Notes

Item	Catalog Number
iCell Cardiomyocytes ² Kit, 01434	R1017
• iCell Cardiomyocytes ² , 01434 ^a	• C1016 (≥5.0 x 10 ⁶ viable cells)
• iCell Cardiomyocytes Plating Medium ^a	• M1001 (30 ml)
• iCell Cardiomyocytes Maintenance Medium ^a	• 2 x M1003 (100 ml)
• iCell Cardiomyocytes ² User's Guide ^a	• X1001
iCell Cardiomyocytes ² Kit, 11713	R1218
• iCell Cardiomyocytes ² , 11713 ^a	• C1233 (≥5.0 x 10 ⁶ viable cells)
• iCell Cardiomyocytes Plating Medium ^a	• M1001 (30 ml)
• iCell Cardiomyocytes Maintenance Medium ^a	• 2 x M1003 (100 ml)
• iCell Cardiomyocytes ² User's Guide ^a	• X1001
Certificate of Analysis ^b	
Certificate of Origin	
If required for shipping purposes	
a Safety Data Sheets and User's Guide available online: www.fujifilmcdi.com/lit/	
b Available online: www.fujifilmcdi.com/coa/	

Required Equipment and Consumables

Item	Vendor(s)	Catalog Number(s)
Equipment		
37°C Water Bath	Multiple Vendors	
Biological Safety Cabinet with UV Lamp	Multiple Vendors	
Cell Culture Incubator	Multiple Vendors	
Hemocytometer or Automated Cell Counter ¹	Multiple Vendors	
Liquid Nitrogen Storage Unit	Multiple Vendors	
Phase Contrast Microscope	Multiple Vendors	
Pipettors	Multiple Vendors	
Tabletop Centrifuge	Multiple Vendors	
Consumables		
0.1% Gelatin in Water ²	STEMCELL Technologies	07903
12-well Flat-bottom Plate, Tissue Culture-treated, Costar	Multiple Vendors	
96-well Flat-bottom Microplate, TC-treated, Falcon	Multiple Vendors	
Conical Tubes, 50 ml, Falcon (Centrifuge Tubes)	Multiple Vendors	
Serological Pipettes, 1, 2, 5, 10, 25 ml	Multiple Vendors	
Sterile Distilled Water	Multiple Vendors	
Trypan Blue ²	Gibco	15250

1 Ensure the automated cell counter is appropriately calibrated before use.

2 Similar products are available from multiple vendors.

Technical Support, Knowledge Base, and Training

FCDI's Technical Support Scientists have the necessary laboratory and analytical experience to respond to your inquiries. Our web-based Knowledge Base provides solutions for iCell related questions about plating and media, cell culture, general assay methods, and more. In addition, in-lab training may be available upon request.

Telephone (877) 320-6688 (US toll-free) / (608) 310-5100 x3
Monday - Friday, 8:30 am - 5:00 pm US Central Time


Fax (608) 310-5101

Email fcdi-support@fujifilm.com

Knowledge Base www.fujifilmcdi.com/knowledgebase/

Workflow Diagram

Notes

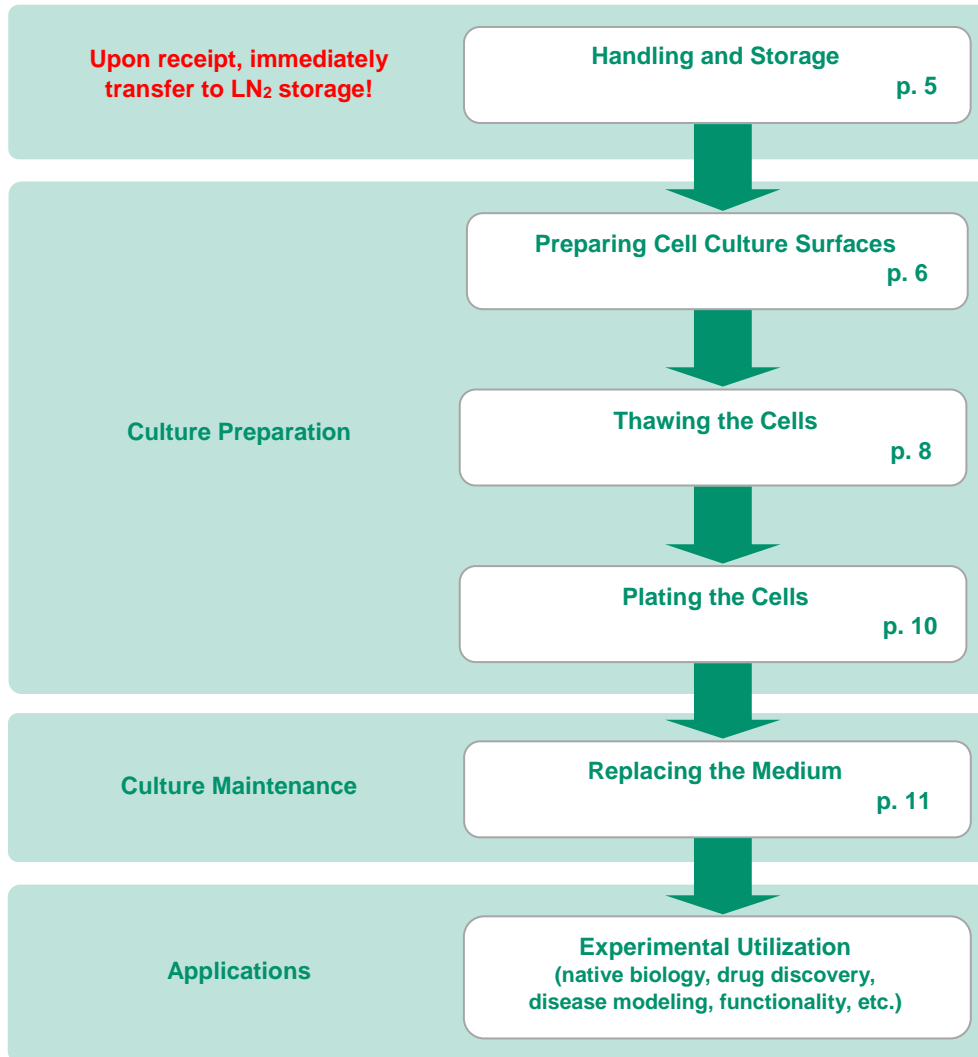

Chapter 2. Handling and Storage

Handling iCell Cardiomyocytes²

iCell Cardiomyocytes² are provided as cryopreserved single-cell suspensions in 1.5 ml cryovials. Upon receipt, directly transfer the cryobox containing iCell Cardiomyocytes² to the vapor phase of a liquid nitrogen storage dewar. FCDI strongly recommends transferring the entire cryobox into the storage rack to avoid transferring individual vials.



It is critical to maintain cryopreserved iCell Cardiomyocytes² at a stable temperature. Minimize exposure of cryopreserved iCell Cardiomyocytes² to ambient temperature when transferring vials to liquid nitrogen storage.

Handling iCell Cardiomyocytes Media

iCell Cardiomyocytes Plating Medium and iCell Cardiomyocytes Maintenance Medium are shipped frozen on dry ice. Upon receipt, store iCell Cardiomyocytes media at -20°C until ready for use and at 4°C for up to 2 weeks post-thawing. If media will be used for longer than 2 weeks, aliquot and freeze again after the initial thaw. Do not subject media to more than a single refreeze and thaw cycle.

Chapter 3. Preparing Cell Culture Surfaces

iCell Cardiomyocytes² will plate and function on a variety of substrates including gelatin or fibronectin, which have been shown to support attachment, viability, and function of iCell Cardiomyocytes² with similar efficiencies. Coating plates with 0.1% gelatin in water is economical, simple, and recommended method for preparing cell culture plates for culturing iCell Cardiomyocytes².

FCDI provides application protocols that recommend assay-specific substrates. See www.fujifilmcdi.com/lit/ for a list of available application protocols for iCell Cardiomyocytes². Regardless of the substrate of choice, prepare plating surfaces before thawing iCell Cardiomyocytes².

1. Select the cell culture vessel appropriate for your experimental use. Add the volume of 0.1% gelatin in water specified in the table below. Scale volumes appropriately for other vessel formats.

Culture Vessel	Surface Area (cm ²)	Volume of 0.1% Gelatin in Water (ml)
12-well Cell Culture Plate	3.8	1.2
96-well Cell Culture Plate	0.32	0.1

Table 1: Summary of Useful Volumes and Measures

All volumes and measures are **per well**, if applicable.

Note: For glass coverslips for immunocytochemistry or electrophysiological applications, see the iCell Cardiomyocytes Application Protocols available online at www.fujifilmcdi.com/lit/.

2. Incubate the vessel(s) in a 37°C cell culture incubator for at least 1 hour.
3. Aspirate the 0.1% gelatin in water immediately before addition of the cell suspension.



Do not allow the gelatin-coated surface to dry.

Chapter 4. Thawing Media

iCell Cardiomyocytes Plating Medium (Plating Medium) and iCell Cardiomyocytes Maintenance Medium (Maintenance Medium) have been specially formulated to maximize the cell viability and recovery at thaw, and to maintain the health and function of iCell Cardiomyocytes² in culture over time, respectively. Thaw and store the media as follows:

1. 24 hours before use, thaw the media overnight at 4°C.
2. Prepare aliquots of media and store at 4°C for up to 2 weeks.

Note: *The medium aliquots can be stored at -20°C. Do not thaw and refreeze the medium aliquots multiple times.*

Chapter 5. Thawing iCell Cardiomyocytes²

Maintain iCell Cardiomyocytes² in liquid nitrogen until immediately before thawing to ensure maximal performance of the cells. Complete the following steps of the thawing procedure in a time-efficient manner to facilitate optimal iCell Cardiomyocytes² viability and performance.

Note: Thaw no more than 3 vials of iCell Cardiomyocytes² at one time.

1. Equilibrate the Plating Medium at room temperature before thawing iCell Cardiomyocytes².
2. Remove the iCell Cardiomyocytes² cryovial from the liquid nitrogen storage tank.

Note: If necessary, place cryovials on dry ice for up to 60 minutes before thawing.

3. Immerse the cryovial in a 37°C water bath for 3 minutes (avoid submerging the cap), holding the tube stationary (no swirling). Use of a floating microcentrifuge tube rack is recommended.



Precise timing is critical to maximizing viable cell recovery.

4. Immediately remove the cryovial from the water bath, spray with 70% ethanol, and place into the biological safety cabinet.
5. Gently transfer the iCell Cardiomyocytes² cryovial contents to a sterile 50 ml centrifuge tube using a 1 ml pipettor.

Note: Use of a 50 ml centrifuge tube facilitates suitable mixing to minimize osmotic shock and increase cardiomyocyte viability.



Avoid repeated pipetting of the thawed iCell Cardiomyocytes² cell suspension.

6. Rinse the empty iCell Cardiomyocytes² cryovial with 1 ml of room temperature Plating Medium to recover any residual cells from the vial.
7. Transfer the 1 ml of Plating Medium rinse from the cryovial drop-wise over 90 seconds (i.e. 1 drop every 4 - 5 seconds) to the 50 ml centrifuge tube containing the iCell Cardiomyocytes² cell suspension. Gently swirl the tube while adding the medium to mix the solution completely and minimize the osmotic shock on the thawed cells.



Drop-wise addition of Plating Medium to the cell suspension is critical to minimize osmotic shock and ensure maximum viability and attachment of the cells to the plating substrate. See the Handling iCell Cardiomyocytes Training Video available online at www.fujifilmcdi.com/cm_handling/ as a reference for the thawing steps only.

8. Slowly add 8 ml of room temperature Plating Medium to the 50 ml centrifuge tube. Add the first 1 ml drop-wise over 30 - 60 seconds. Then add the

Notes

remaining volume over the next ~30 seconds. Gently swirl the centrifuge tube while adding the medium.



It is critical to add the Plating Medium slowly to ensure maximum viability and attachment of the cells once plated.

9. Gently mix the contents of the 50 ml centrifuge tube by inverting 2 - 3 times. Gentle mixing is critical to ensure maximum viability. Avoid vigorous shaking or vortexing of the cell suspension.

Note: *Thaw up to 3 vials of iCell Cardiomyocytes² at one time. Once thawed, you can pool the contents of the vials before adding the rinse and final volume of Plating Medium. Follow the timing outlined in steps 6 and 7. For example, if pooling 3 vials, add each 1 ml of rinse over 90 seconds (270 seconds total).*

Chapter 6. Plating iCell Cardiomyocytes²

The recommended seeding density for iCell Cardiomyocytes² in standard cell culture plates is 156,000 viable cells/cm². For application-specific plating instructions, see the Application Protocols available online at www.fujifilmcdi.com/lit/.

1. Obtain the number of viable cells/vial and viability from the Certificate of Analysis.
1. Invert the thawed iCell Cardiomyocytes² cell suspension 2 - 3 times to ensure an even cardiomyocyte distribution before performing the cell count.
2. Remove a sample of cells to confirm viability using a hemocytometer (using trypan blue exclusion to identify viable cells) or an automated cell counter.
3. Calculate the final volume of room temperature Plating Medium needed to obtain a desired cell plating density (i.e., 5×10^5 cells/ml) using the number of viable cells/vial from the Certificate of Analysis. See Table 2 below for examples.

Note: If your application requires higher cell densities, centrifuge iCell Cardiomyocytes² at 180 x g for 5 minutes, remove the necessary amount of the Plating Medium to achieve the desired density, and gently resuspend the iCell Cardiomyocytes² pellet. Note that over-pipetting could reduce cell viability.

Culture Vessel	Surface Area (cm ²)	Plating Volume (ml)	Cell Number (1.56×10^5 cells/cm ²)
12-well Cell Culture Plate	3.8	1.2	593×10^3
96-well Cell Culture Plate	0.32	0.1	50×10^3

Table 2: Summary of Recommended Volumes and Measures

This table provides a guide for syncytial formation only. All volumes and measures are per well unless otherwise indicated.

4. Aspirate the 0.1% gelatin in water from the pre-coated cell culture vessel(s).
5. Invert the cell suspension 2 - 3 times and immediately dispense the cell suspension into the pre-coated cell culture vessel(s).
6. Culture iCell Cardiomyocytes² in a cell culture incubator at 37°C, 5% CO₂ **for 4 hours**. Proceed immediately to Chapter 7, Maintaining iCell Cardiomyocytes².

Chapter 7. Maintaining iCell Cardiomyocytes²

1. Immediately before use, equilibrate iCell Cardiomyocytes Maintenance Medium (Maintenance Medium) in a 37°C water bath.
2. 4 hours post-plating iCell Cardiomyocytes², aspirate the Plating Medium using a pipettor and replace with the appropriate volume of Maintenance Medium. Be careful not to touch or disrupt the adhered cardiomyocytes.
3. Replace the Maintenance Medium every other day.
4. Culture iCell Cardiomyocytes² in a cell culture incubator at 37°C, 5% CO₂.



iCell Cardiomyocytes², 01434 are ready to assay on day 4 post-plating, whereas iCell Cardiomyocytes², 11713 are ready to assay on day 7 post-plating.

The cells are FOR RESEARCH USE ONLY and NOT FOR THERAPEUTIC USE. See www.fujifilmcdi.com/product-warranty/ for USE RESTRICTIONS applicable to the cells and other terms and conditions related to the cells and their use.

© 2018 FUJIFILM Cellular Dynamics, Inc. All rights reserved.